



MODEL 3340 G-LOGGER

DATA ACQUISITION SYSTEM

Silicon Designs ISD

• Start and stop data acquisitions with button and/or schedule

- Collect information on peak
- View a list of peak events and event data in any display mode
- Add a GPS module to also collect GPS data •
- Uses internal battery power, external power packs or AC power
- Compatible with Silicon Designs accelerometers •
- Automatic and manual calibration routines via +/-1G flip
- Adjustable filters and FFT for live or post collection data • analysis
- Included software features familiar and convenient user • interface built on a LabView platform
- Three input channels for three 1- axis modules or one 3-axis • module
- 16-bit sample rates from 1 to 10,000 samples/second per axis
- Automatic setup in less than 5 minutes upon wiring of Silicon Designs accelerometer modules

25 Pin Female D-Sub

Micro USB (B)

32 GB



SPECIFICATIONS

PHYSICAL

Case Size Weight Case Material

OPERATIONAL

USB Connection

Max SD Card Size

Memory Type

Connection

5.5" x 4.25" x 2.5" 425 grams / 15 oz. + batteries Die Cast Aluminum, Plastic

ENVIRONMENTAL Operating Temperature Storage Temperature Humidity

PC REQUIREMENTS

Operating Systems Host Connection SD Card, Micro SD w/ Adaptor Power Supply Max Power Consumption TCP/IP Remote Operation $0^{\circ}C$ to $+55^{\circ}C$ (max) -40°C to +85°C (max) 0% - 90% Non-condensing

Windows 10, 8, 7, XP USB2 Type A USB/AC Power/AA Batteries 750 mW Network Connection Req.

ICATIONS TO MEDIUM FREQI



ADDITIONAL FEATURES

• Real time data monitoring

- Collect data in G or volts
- Display shows from 100ms to 2 minutes of data
- FFT (Fast Fourier Transform) analysis is an advanced feature usually found on much more expensive DAQ systems
- Independent scale G/Div settings expand or shrink each channel's input for better visibility
- PAUSE, RWD, FWD without interrupting data
- Optional offsets provide a staggered display for no overlap
- Independent scale G/Div per channel
- Oscilloscope (Sweep, Scope, Strip) and Volt Meter modes
- Hide or show any or all of the 3 channels
- View data from remote locations on network via TCP/IP
- Optional offset setting per channel
- Export time-stamped data to Excel, MatLab etc.


collection

Silicon Designs, Inc. • 13905 NE 128th Street, Kirkland WA 98034 • Phone: 425-391-8329 • Fax: 425-391-0446




DATA COLLECTION

Data can be collected live or recorded for playback later. Modifying the horizontal scale expands or contracts the period of time displayed on the screen from 100ms up to 2 minutes. Each axis is one channel, and these can be hidden or offset (but will still be recorded) as desired.

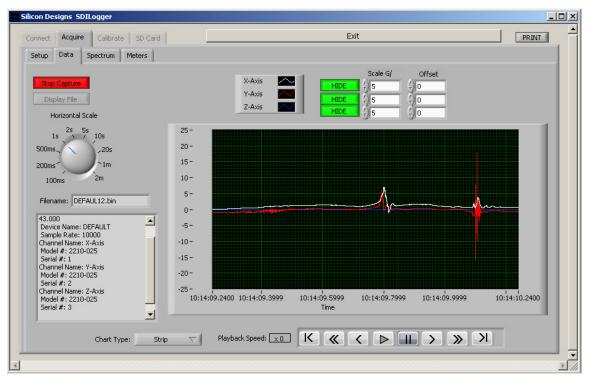

SPECTRUM (FFT)

SPECTRUM displays the FFT of the data. This is a more advanced feature of the G-logger 3340. You can analyze the data to see at which frequencies the maximum vibrations are occurring.

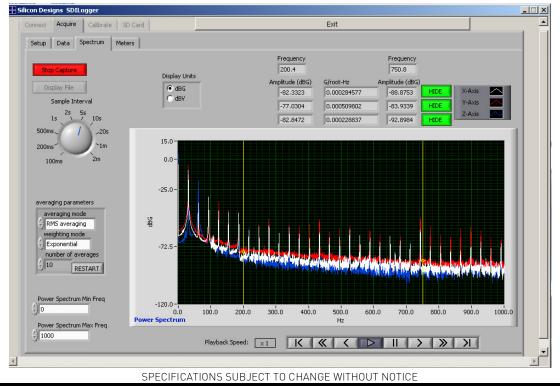


Silicon Designs, Inc. • 13905 NE 128th Street, Kirkland WA 98034 • Phone: 425-391-8329 • Fax: 425-391-0446




PEAK VALUES

The METERS screen provides DC, RMS, and peak values in either Volts or Gs. These values are calculated over the time interval selected by the horizontal scale selected on the Data tab. The values are updated at that same interval as well.

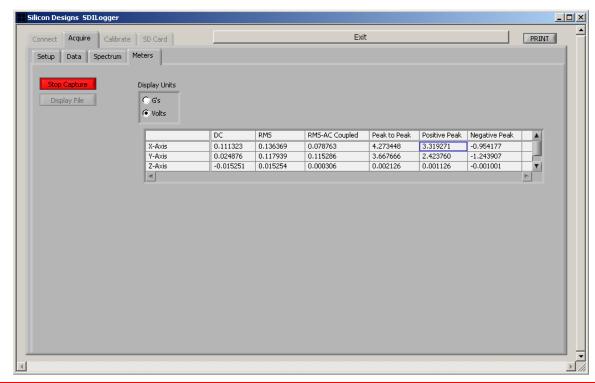

CALIBRATE

The default calibration parameters are supplied automatically, or unit-specific calibration parameters can be manually entered. Manual calibration can be done any time using gravity and performing a simple +/-1G flip.

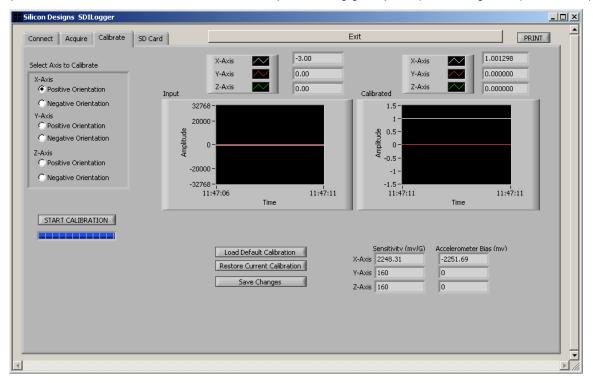

SPECIFICATIONS SUBJECT TO CHANGE WITHOUT NOTICE

Silicon Designs, Inc. • 13905 NE 128th Street, Kirkland WA 98034 • Phone: 425-391-8329 • Fax: 425-391-0446



PEAK EVENT REPORTING


When event detection is enabled, the 3340 will identify and write events whenever data acquisition occurs. The peak events are written to a file on the SD card, which is then automatically specified as the event file upon saving.

onnect Acquire Calibrate :	SD Card	Exit				
Setup Data Spectrum Met					PRINT	
becap baca spectrum met						
	Events					
	Time	Channel	Magnitude 🔺			
	4/22/2014 12:54:30		0.310698			
	4/22/2014 12:54:31	.0693 Y-Axis	2.420865			
	4/22/2014 12:54:31		-0.038691			
	4/22/2014 12:54:31		2.090497			
	4/22/2014 12:54:31		-1.755543			
	4/22/2014 12:54:31		2.281478			
	4/22/2014 12:54:31	L.9949 Y-Axis	-2.418054			
	4/22/2014 12:54:32	2.0305 Y-Axis	1.954463			
	4/22/2014 12:54:32	2.1562 Z-Axis	-0.060252			
	4/22/2014 12:54:32	2.1617 Z-Axis	2.339380			
	4/22/2014 12:54:32	2.1410 Y-Axis	-2.398621			
	4/22/2014 12:54:32	2.2578 Z-Axis	1.071339			
	4/22/2014 12:54:32	2.2760 Z-Axis	-1.386422			
	4/22/2014 12:54:32	2.2782 Z-Axis	1.539807			
	4/22/2014 12:54:32	2.2830 Z-Axis	2.163923			
	4/22/2014 12:54:32	2.3329 Y-Axis	-1.137195			
	4/22/2014 12:54:33	3.0465 Y-Axis	-2.262587			
	4/22/2014 12:54:33	3.0907 Z-Axis	1.909919 🗾			
	•					

CONNECTOR PIN LAYOUT

TOP ROW	' PIN NUME	BERS										
1	2	3	4	5	6	7	8	9	10	11	12	13
CH 0 0 Volt	CH 0 AON	CH 1 0 Volt	CH 1 AON	CH 2 0 Volt	CH 2 AON	Х	Х	Х	Х	Х	Х	Х
Bottom R	ow Pin Nur	nbers										
14	15	16	17	18	19	20	21	22	23	3	24	25
CH 0 AOP	CH 0 8-32 V	CH 1 AOP	CH 1 8-32 V	CH 2 AOP	CH 2 8-32 V	Х	Х	Х	Х		Х	Х

Included 25 Pin D-Sub Connector for Accelerometer Connection



4





Micro-B

SPECIFICATIONS SUBJECT TO CHANGE WITHOUT NOTICE






Instrument Expert Original factory packaging www.dorgean.com

III SDI

MODEL 3340 G-LOGGER

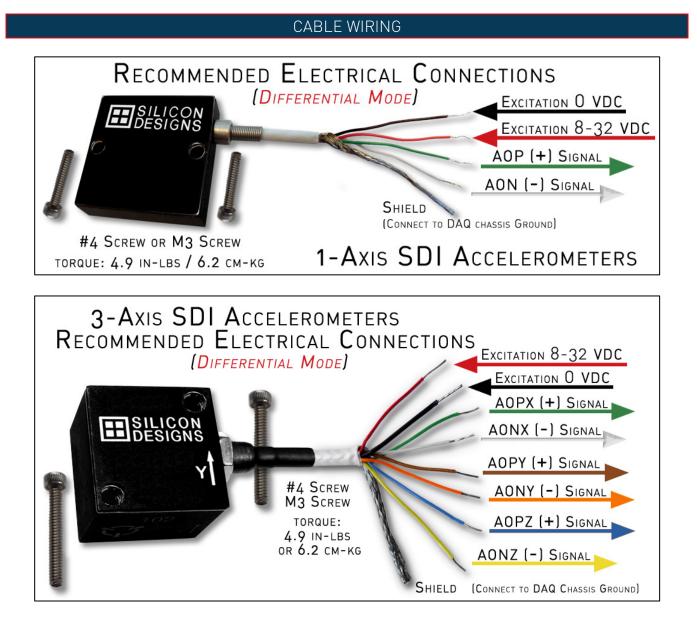

SPECIFICATIONS SUBJECT TO CHANGE WITHOUT NOTICE